

FIG. 1

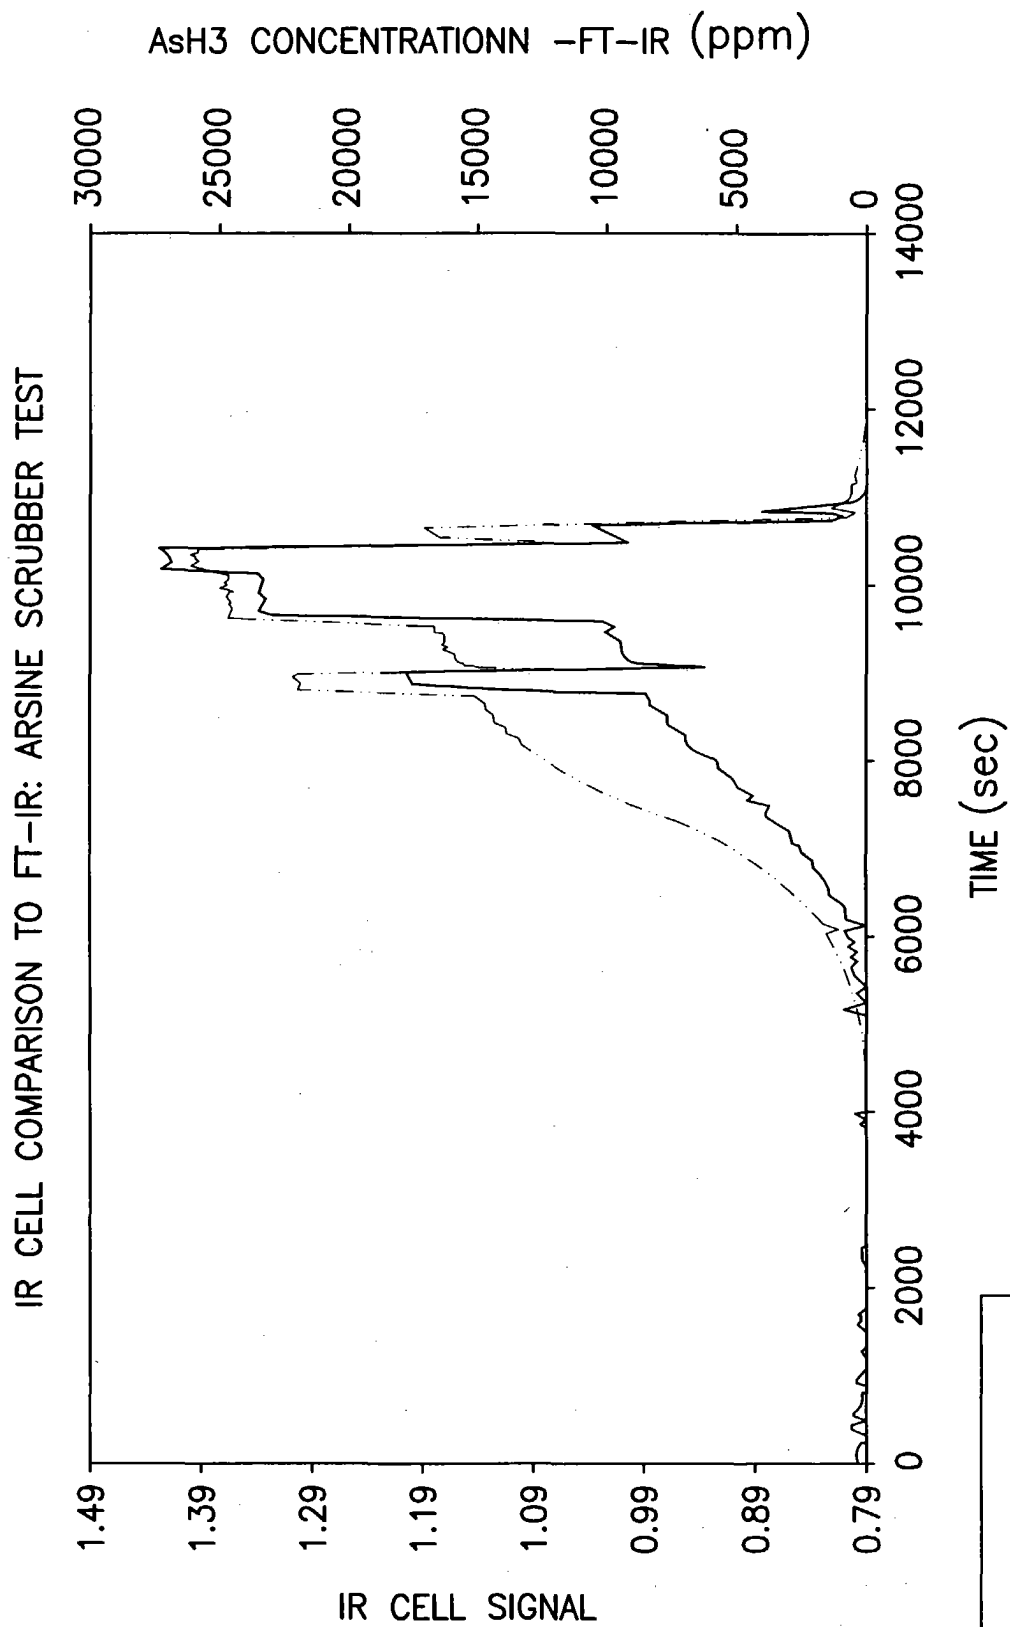


FIG.2

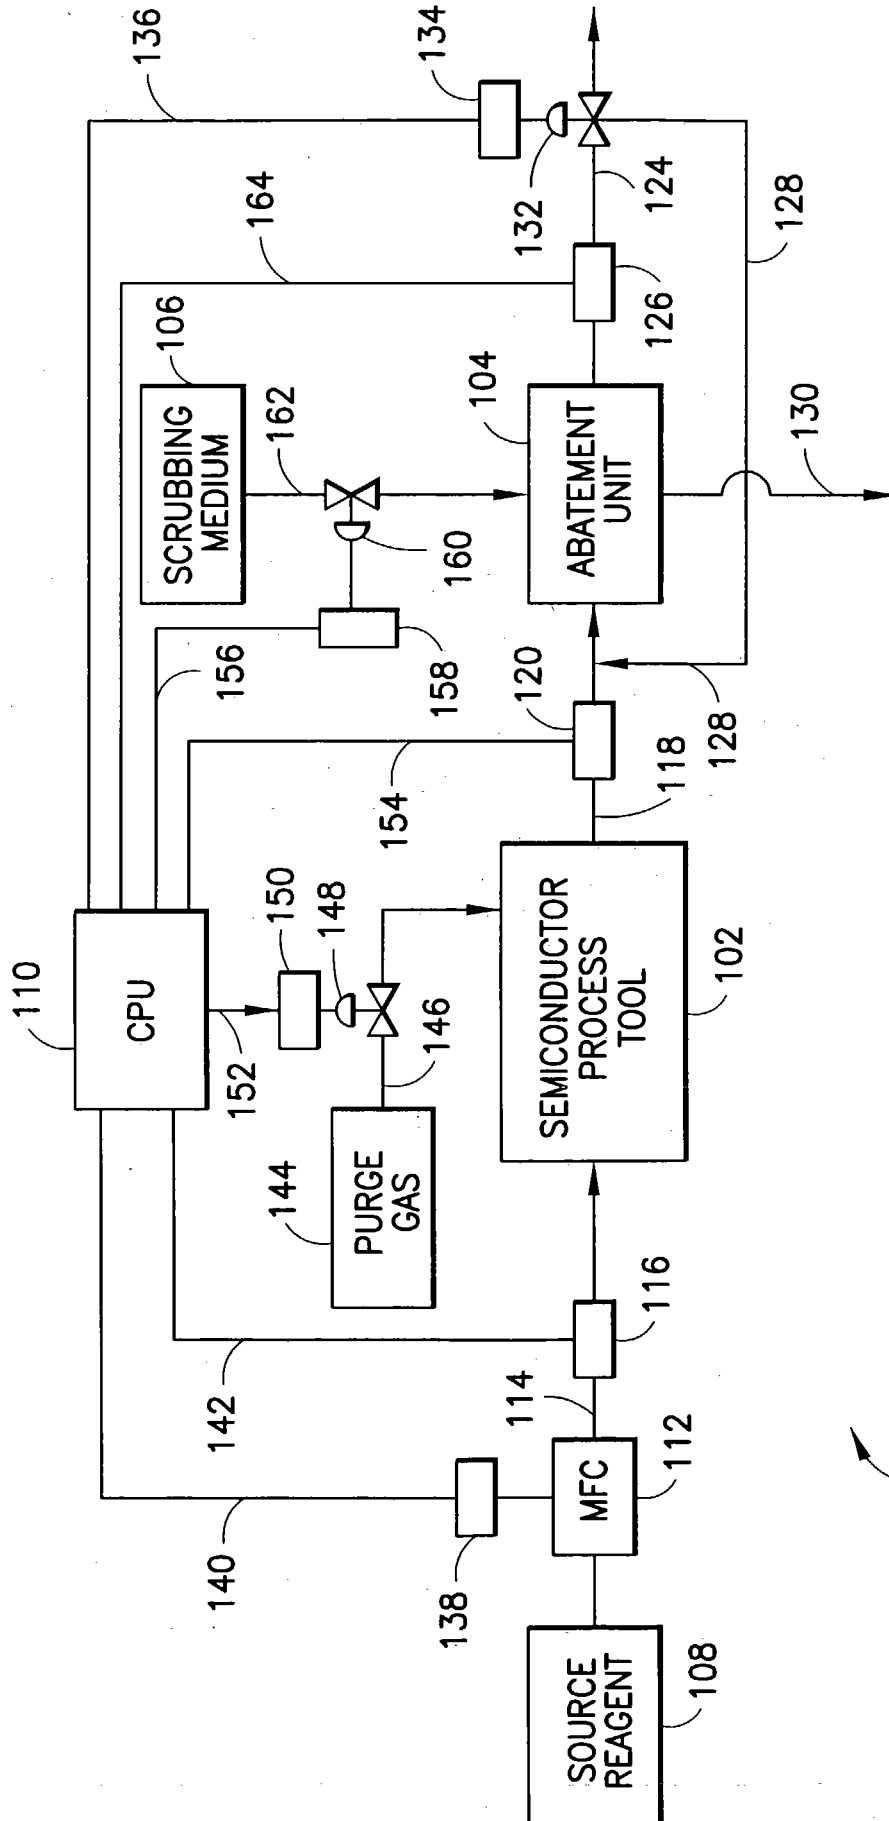


FIG.3

TIME DEPENDENT RESPONSE OF TP MONITOR WITH CHANGING
3MS CONCENTRATIONS

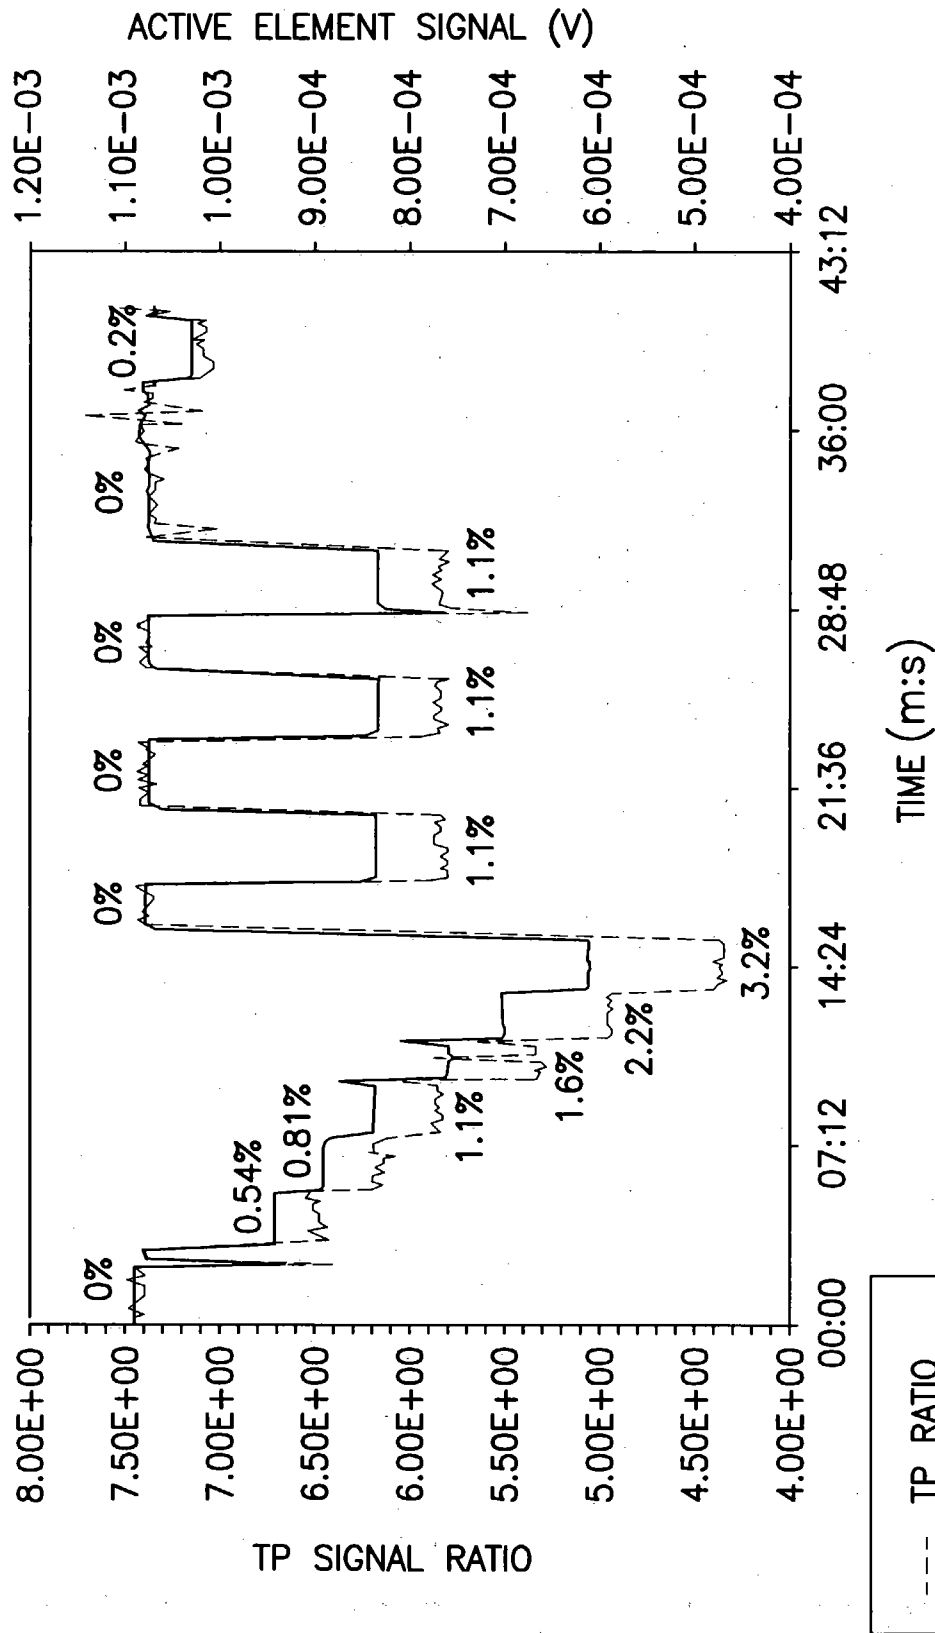


FIG.4

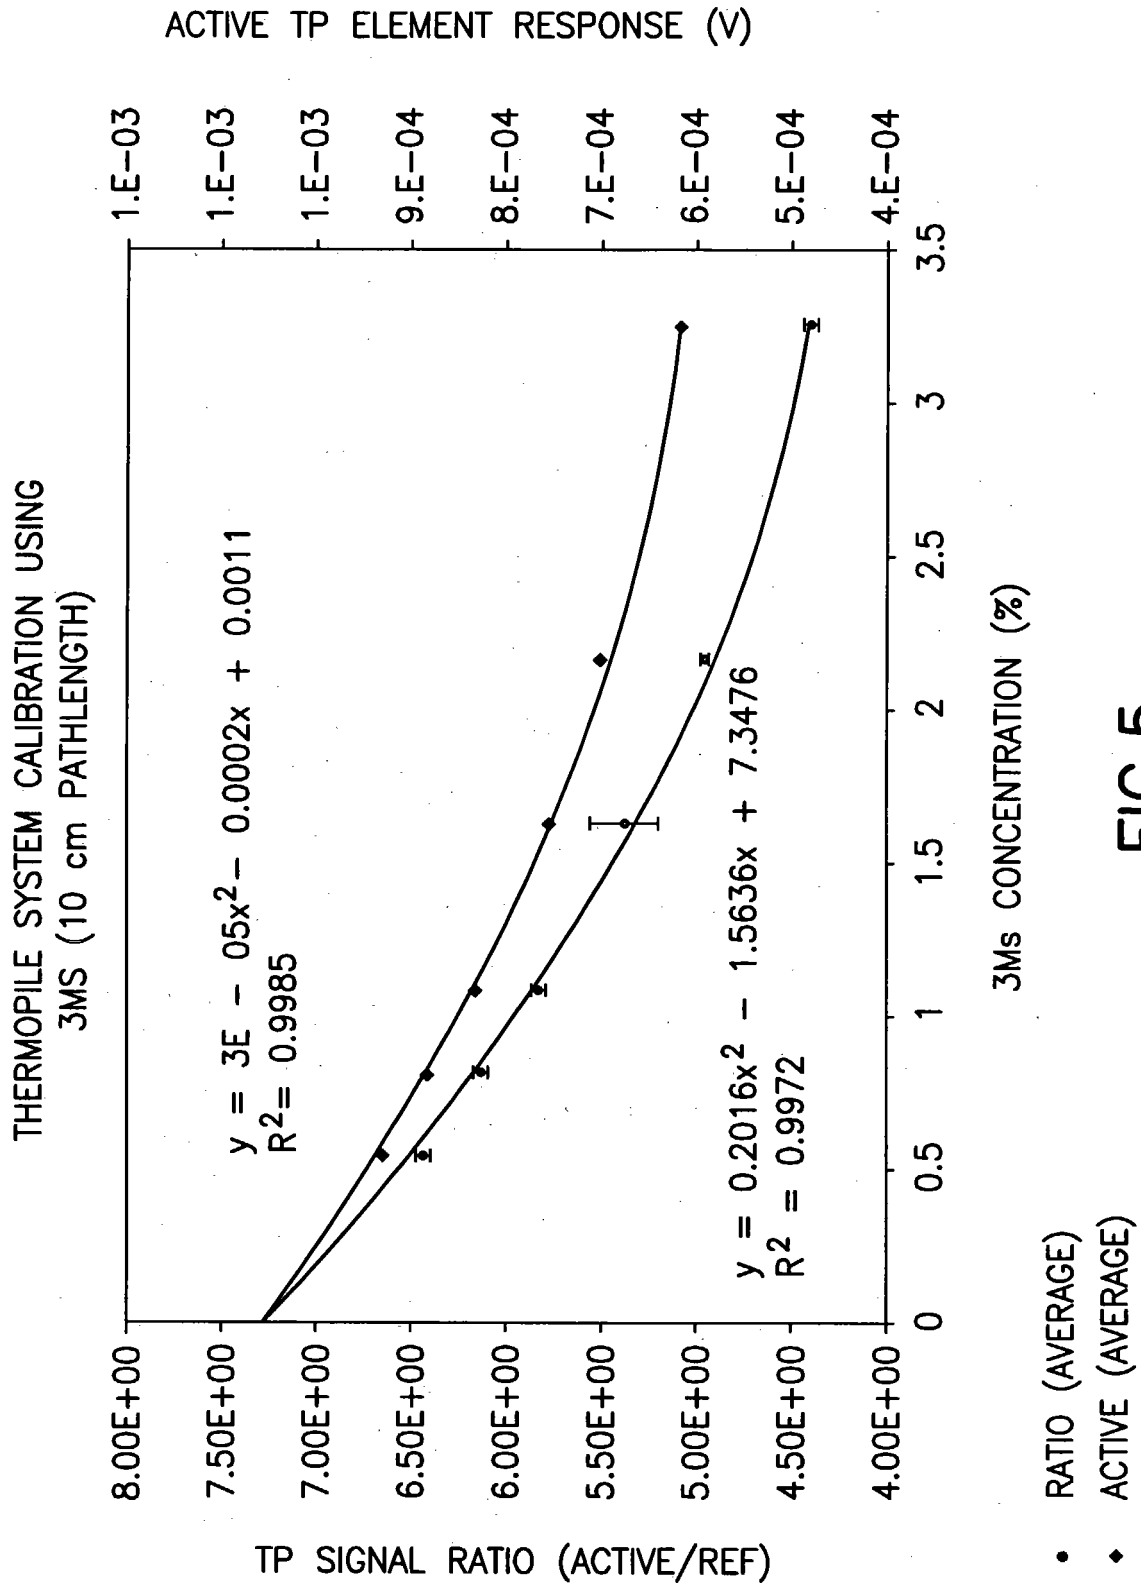


FIG.5